

LDB100F Brightfield LED

LED Illumination Systems for Brightfield Microscopy with Flip-in 550 Nanometer Filter



LDB100F Brightfield LED with flip-in 550 nanometer filter.



Prior Scientific is proud to announce the latest addition to their wide range of illumination products for microscopy - the new Brightfield LED. The Brightfield LED illuminator provides all the advantages of LED illumination in a flexible package that can be fitted to most modern upright and inverted microscope systems.

Brightfield LDB550 features:

- 10,000+ hours of operating lifetime
- <140 microseconds on/off speed using TTL
- LED simply replaces the standard lamphouse
- Internal flip in blocking filter (550 nm LP)
- Eliminates the need for transmitted light shutter
- Small controller for intensity control and on/off control
- Filter in for fluorescence applications eliminating unwanted background fluorescence
- Filter out for brightfield applications, full spectrum
- Higher power for phase contrast and DIC
- Even and constant color temperature illumination
- Powered via Prior ProScan/OptiScan or via stand alone power supply
- Compatible with Nikon Elements

General Specifications:


- 10,000 hours operating lifetime
- Fits most modern upright and inverted microscope systems
- Replaces standard lamphouses
- Choose between manual intensity, TTL control or on/off which eliminates the need for shutter mechanisms

- Compatible with ProScan and OptiScan controllers
- Adapters are available for most modern microscopes
- Can be utilized as a stand alone light source
- <140 microseconds on/off speed using TTL

LDB100F Brightfield LED

LED Illumination Systems for Brightfield Microscopy with Flip-in 550 Nanometer Filter

Brightfield LED Performance Spectrum

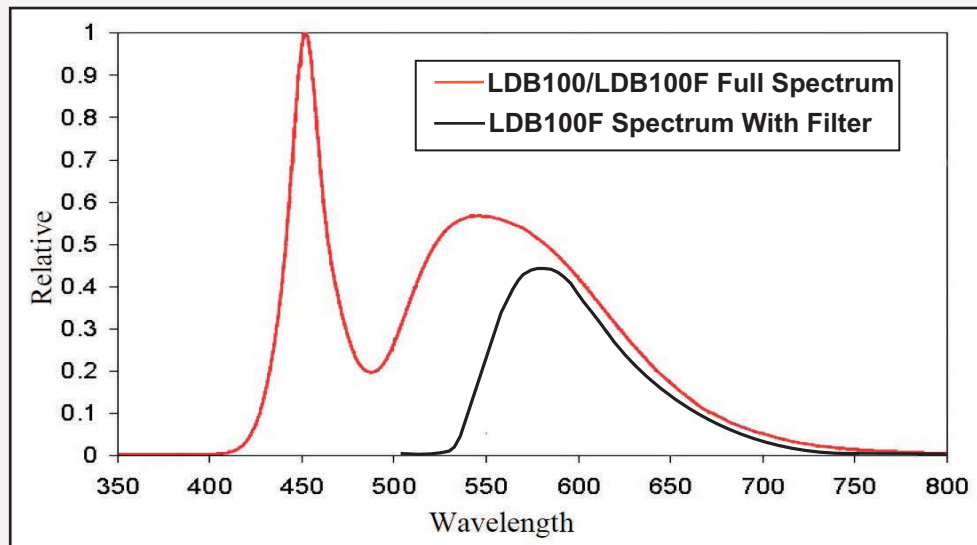

Brightfield LED Ordering Information

Part Number	Description
LDB100FLC*	Brightfield LED with manual flip-in blocking filter for Leica microscopes for use with Prior controller
LDB101FLC	Brightfield LED with manual flip-in blocking filter for Leica microscopes with stand alone power supply
LDB100FNI*	Brightfield LED with manual flip-in blocking filter for Nikon microscopes for use with Prior controller
LDB101FNI	Brightfield LED with manual flip-in blocking filter for Nikon microscopes with stand alone power supply
LDB100FOL*	Brightfield LED with manual flip-in blocking filter for Olympus microscopes for use with Prior controller
LDB101FOL	Brightfield LED with manual flip-in blocking filter for Olympus microscopes with stand alone power supply
LDB100FZS*	Brightfield LED with manual flip-in blocking filter for Zeiss microscopes for use with Prior controller
LDB101FZS	Brightfield LED with manual flip-in blocking filter for Zeiss microscopes with stand alone power supply

*LDB100F units require a compatible Prior controller such as H31XYZEF/H31ZFE or OptiScan controller

Brightfield LED Compatibility Information

Part Number	Description
H31XYZEF	ProScan III controller with X, Y, Z drives, three filter wheel drives and three shutter drives.
H31ZEF	ProScan III controller with three drives for Z focus and two or three filter wheels (includes three shutter drives).
LDBUSBTTL	USB to TTL converter. Emulates ProScan shutter only controller. Requires LDB101 model.
H31ADF	Supplementary module for H31 controller to add three additional filter wheels.
ES100	OptiScan II controller with X, Y, Z drives, two filter wheel drives and three shutter drives.

Worldwide distribution

Prior Scientific, Ltd
Cambridge, UK

Prior Scientific, Inc
Rockland, MA, USA

Prior Scientific, GmbH
Jena, Germany

Prior Scientific KK
Tokyo, Japan

T. +44 (0) 1223 881711
E. uksales@prior.com

T. +1 781-878-8442
E. info@prior.com

T. +49 (0) 3641 675 650
E. jena@prior.com

T. +81-3-5652-8831
E. info-japan@prior.com

